

Contact Lenses for Real-Time Colorimetric Sensing of Glucose

Danielle Bruen^{*1}, Rami Albatal², Larisa Florea¹ and Dermot Diamond¹

¹Insight Centre for Data Analytics, National Centre for Sensor Research, School of Chemical Sciences, Dublin City University, Dublin 9, Ireland.

²Insight Centre for Data Analytics, Dublin City University, Dublin 9, Ireland.


Centre for
Data Analytics




Introduction

Boronic acids (BA) are well-known for their interactions with diol-containing compounds like glucose. Fluorescent moieties are commonly incorporated into a BA derivative's framework to monitor the effect of increased glucose concentrations in a given environment. In this study, a novel carboxylic acid BA derivative, *o*-COOHBA, has been synthesized and investigated for glucose sensing, in solution and when immobilised onto a polydimethylsiloxane (PDMS) "lens"-like surface. In both cases on increased glucose concentrations, a decrease in fluorescence intensity was observed in the range of 0-10mM in solution and similarly, in the range of 0-5mM when anchored to a PDMS surface, corresponding to the ocular-glucose concentrations for diabetics (~500μM – 5mM). This approach aims to develop smart contact lenses that will allow people suffering from diabetes to track their condition non-invasively.

Sensing Mechanism

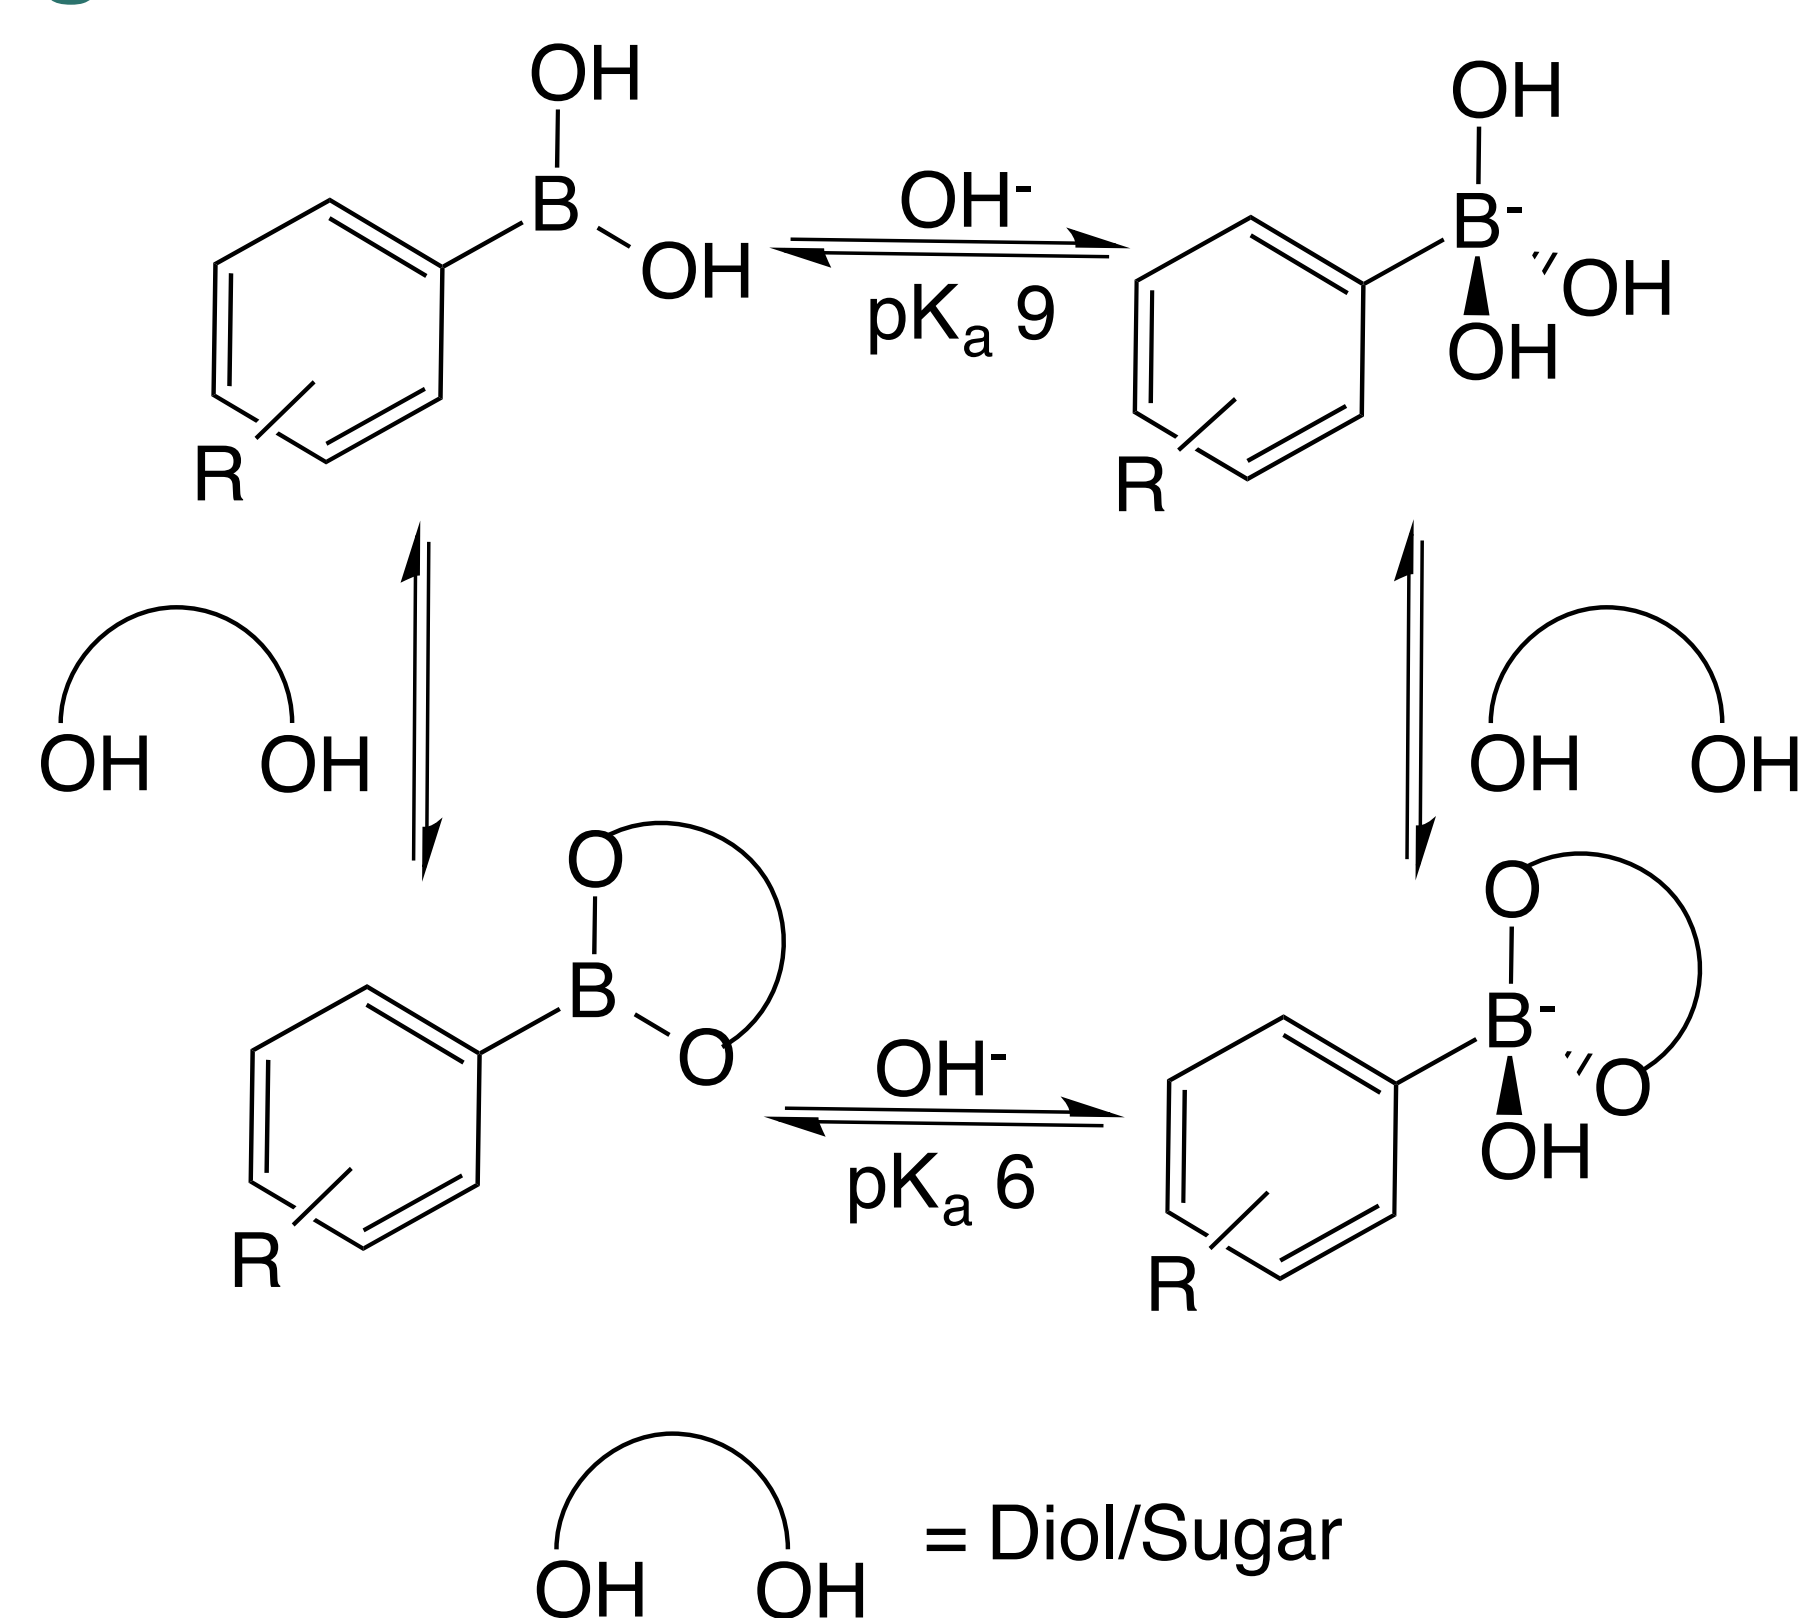


Synthesis of BA Sensor

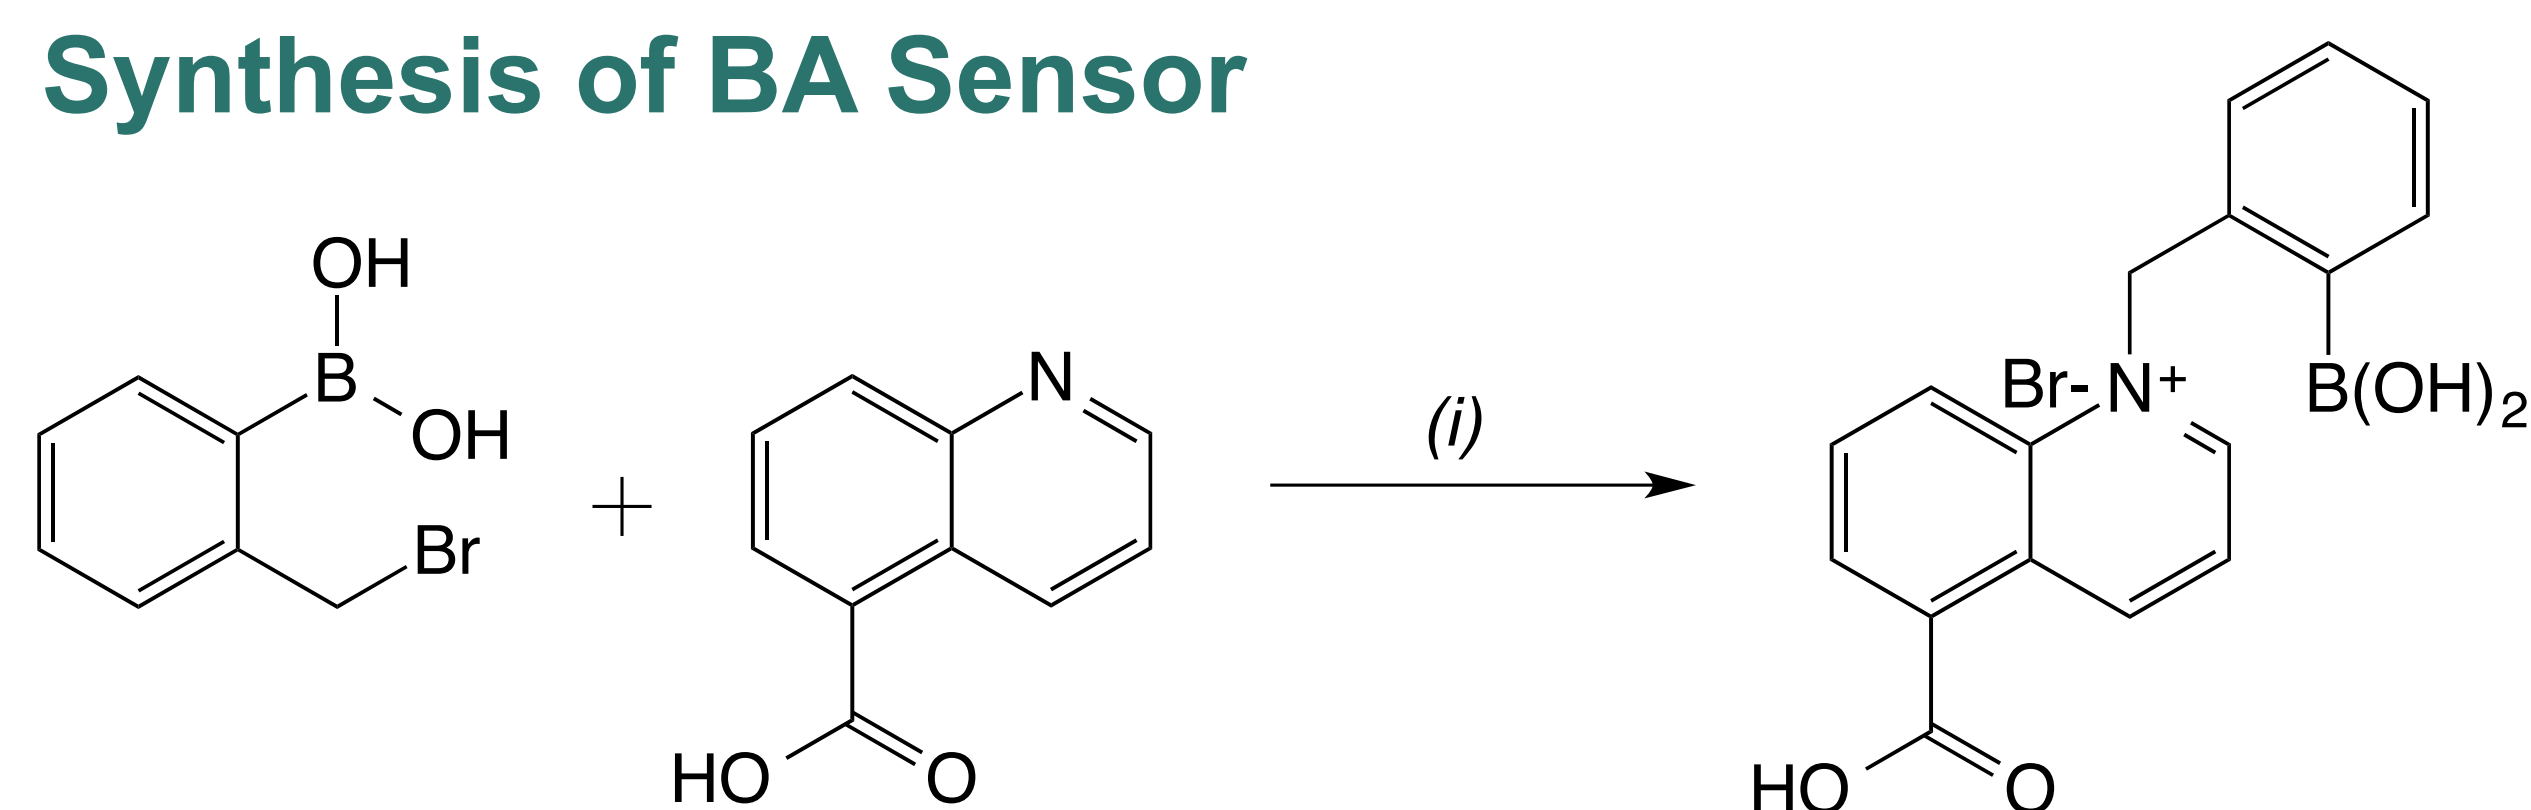

Synthesis of *o*-COOHBA; (i) anhydrous dimethylsulfoxide, N₂, 70 °C for 48h. Formation of *o*-COOHBA was confirmed by ¹H NMR.


PDMS Lens Fabrication

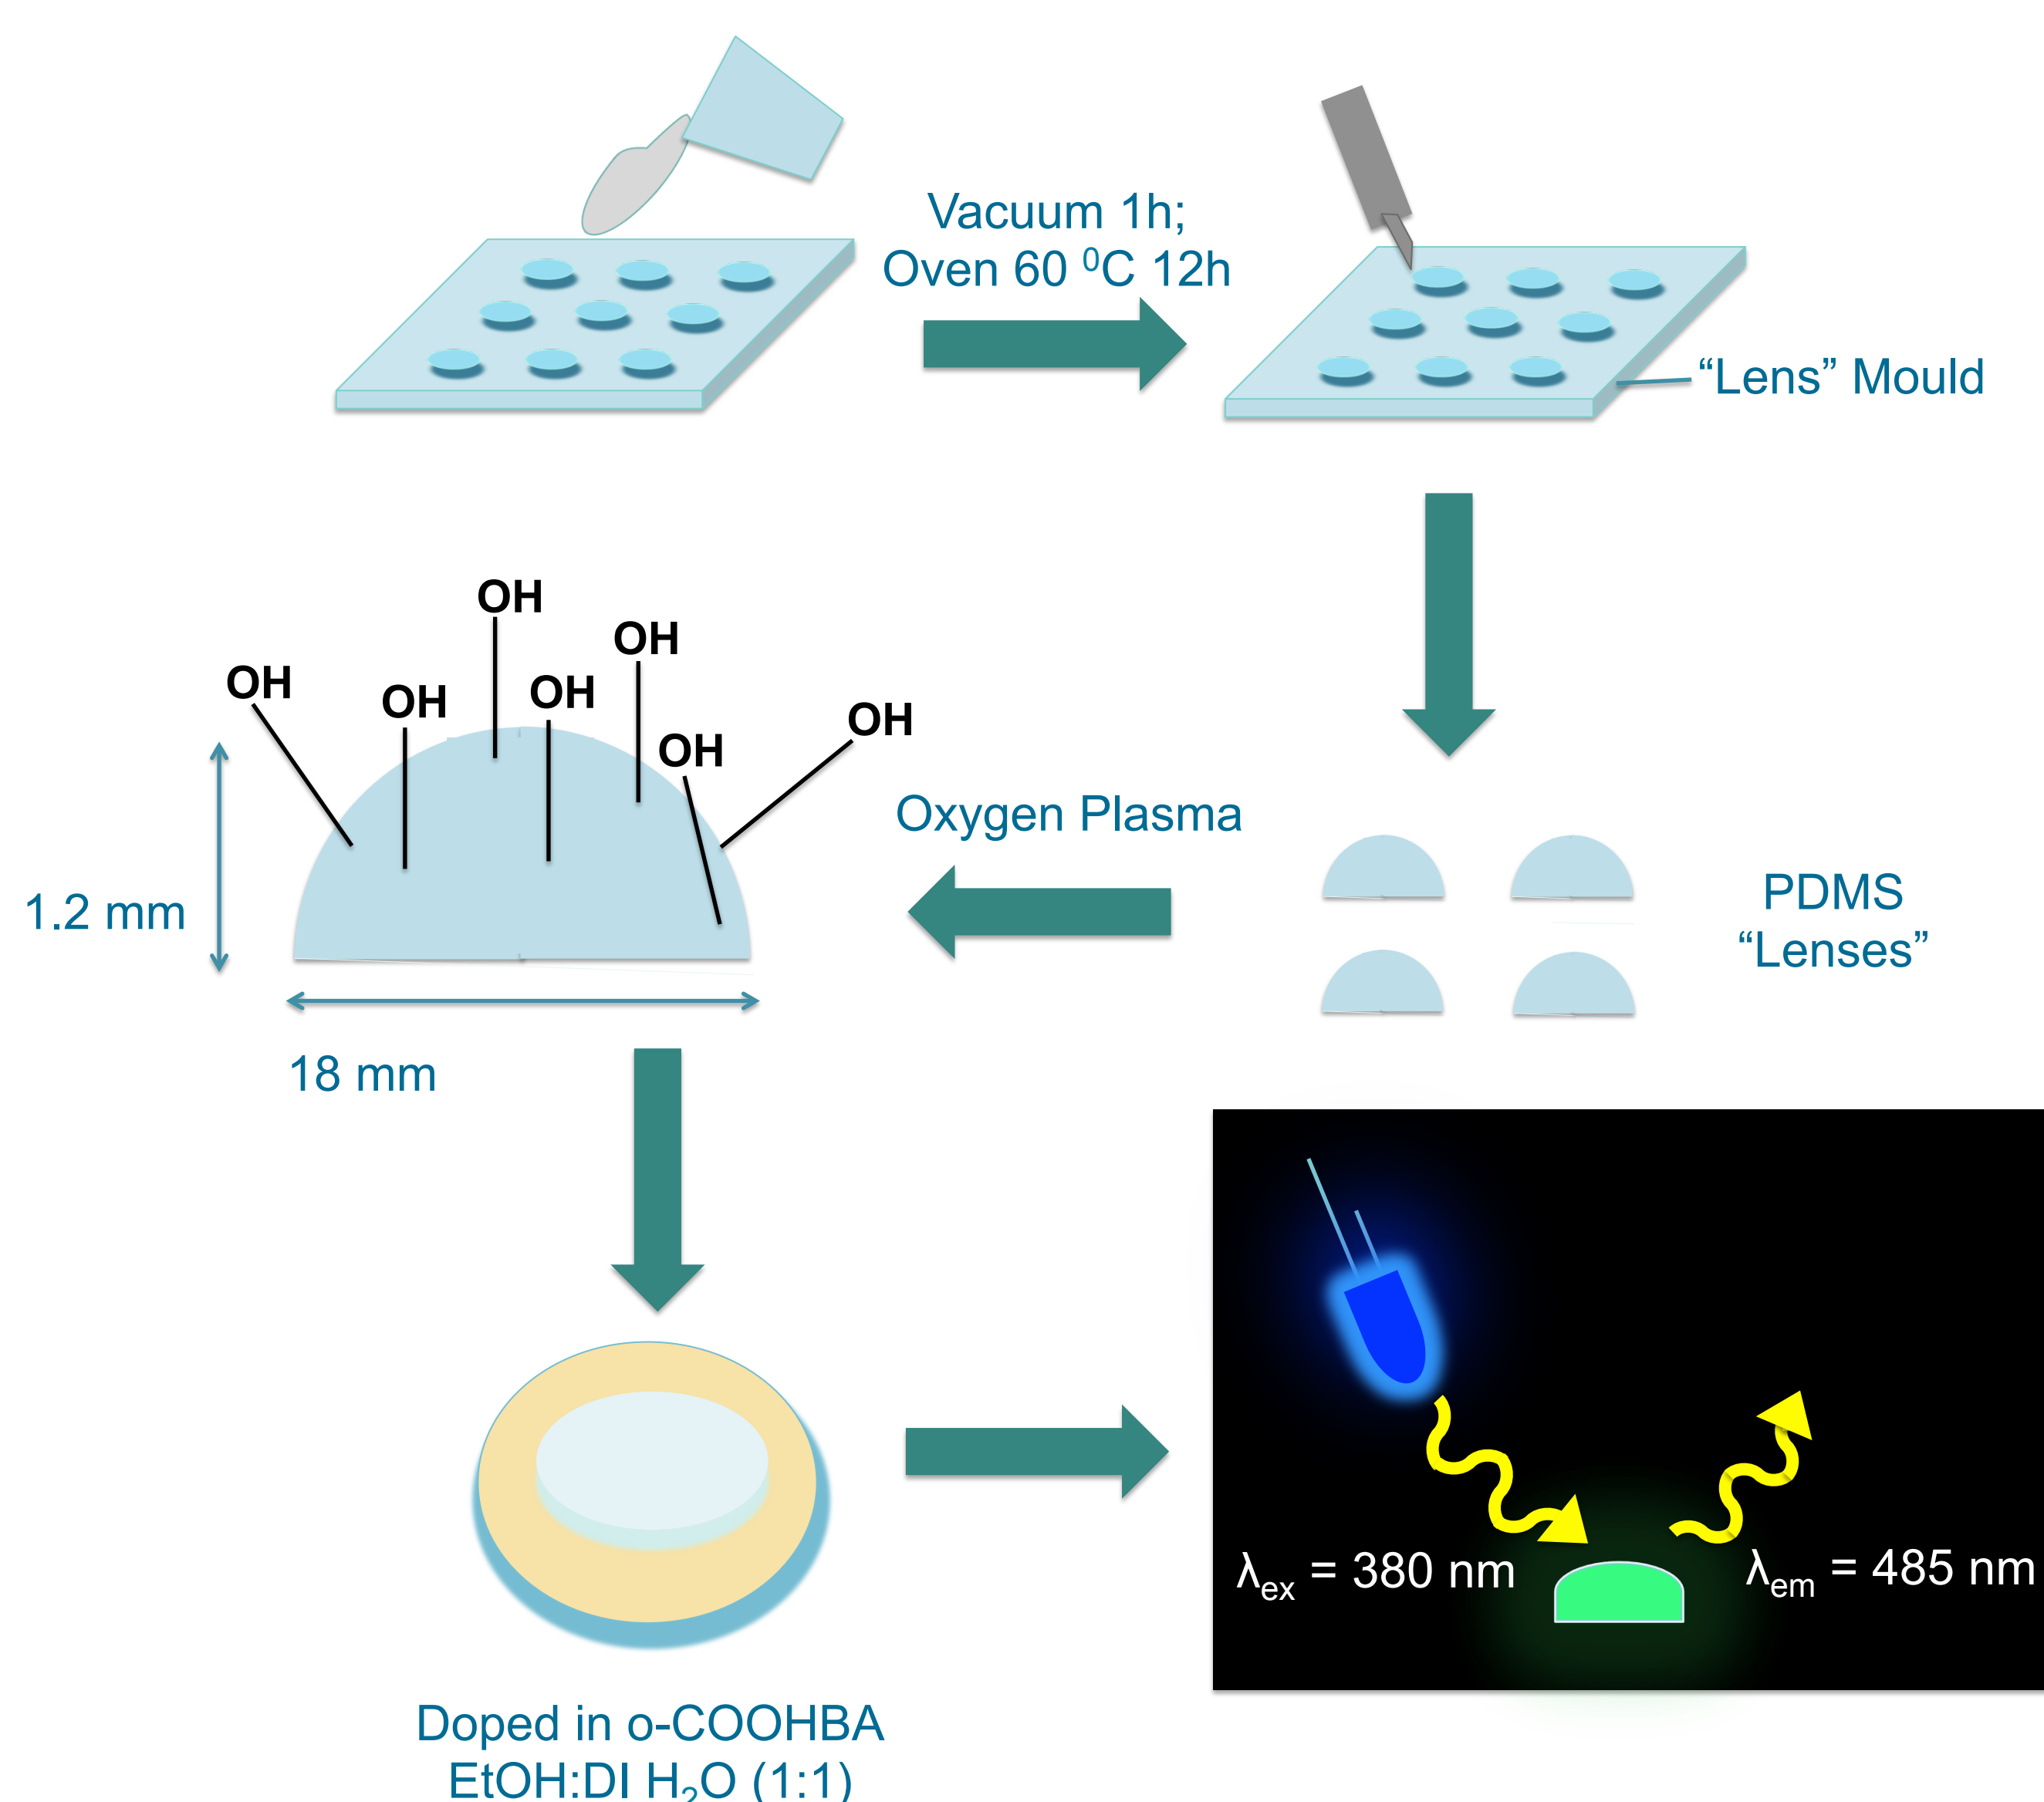

Glucose Sensing

The fluorescence of *o*-COOHBA has been studied in solution and when anchored to a PDMS surface. *o*-COOHBA has shown to respond to glucose in the dynamic range of 0-10mM, which corresponds to the ocular-glucose concentration range in diabetics (~500μM – 5mM).


o-COOHBA in Solution

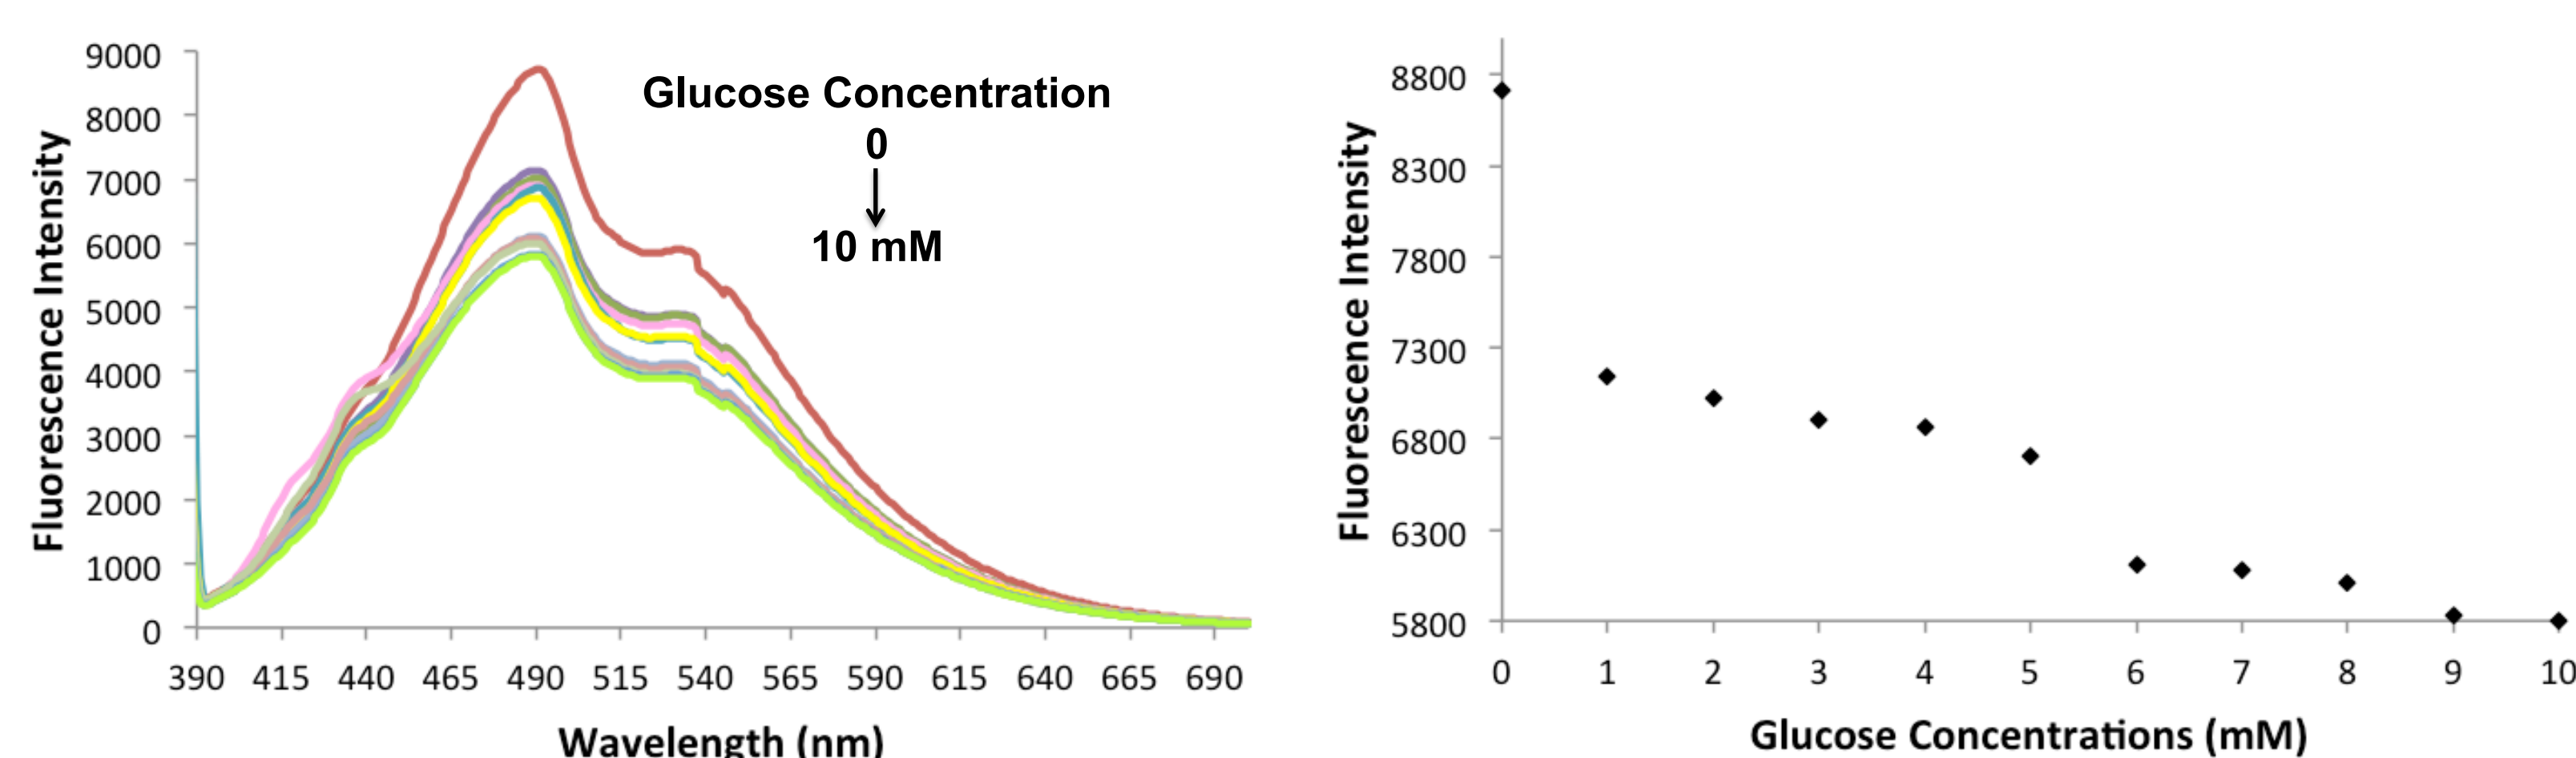

o-COOHBA; 0.5mM in pH 7.4 phosphate buffer

Excitation wavelength 380 nm; Emission wavelength: 485 nm

o-COOHBA Immobilized onto PDMS

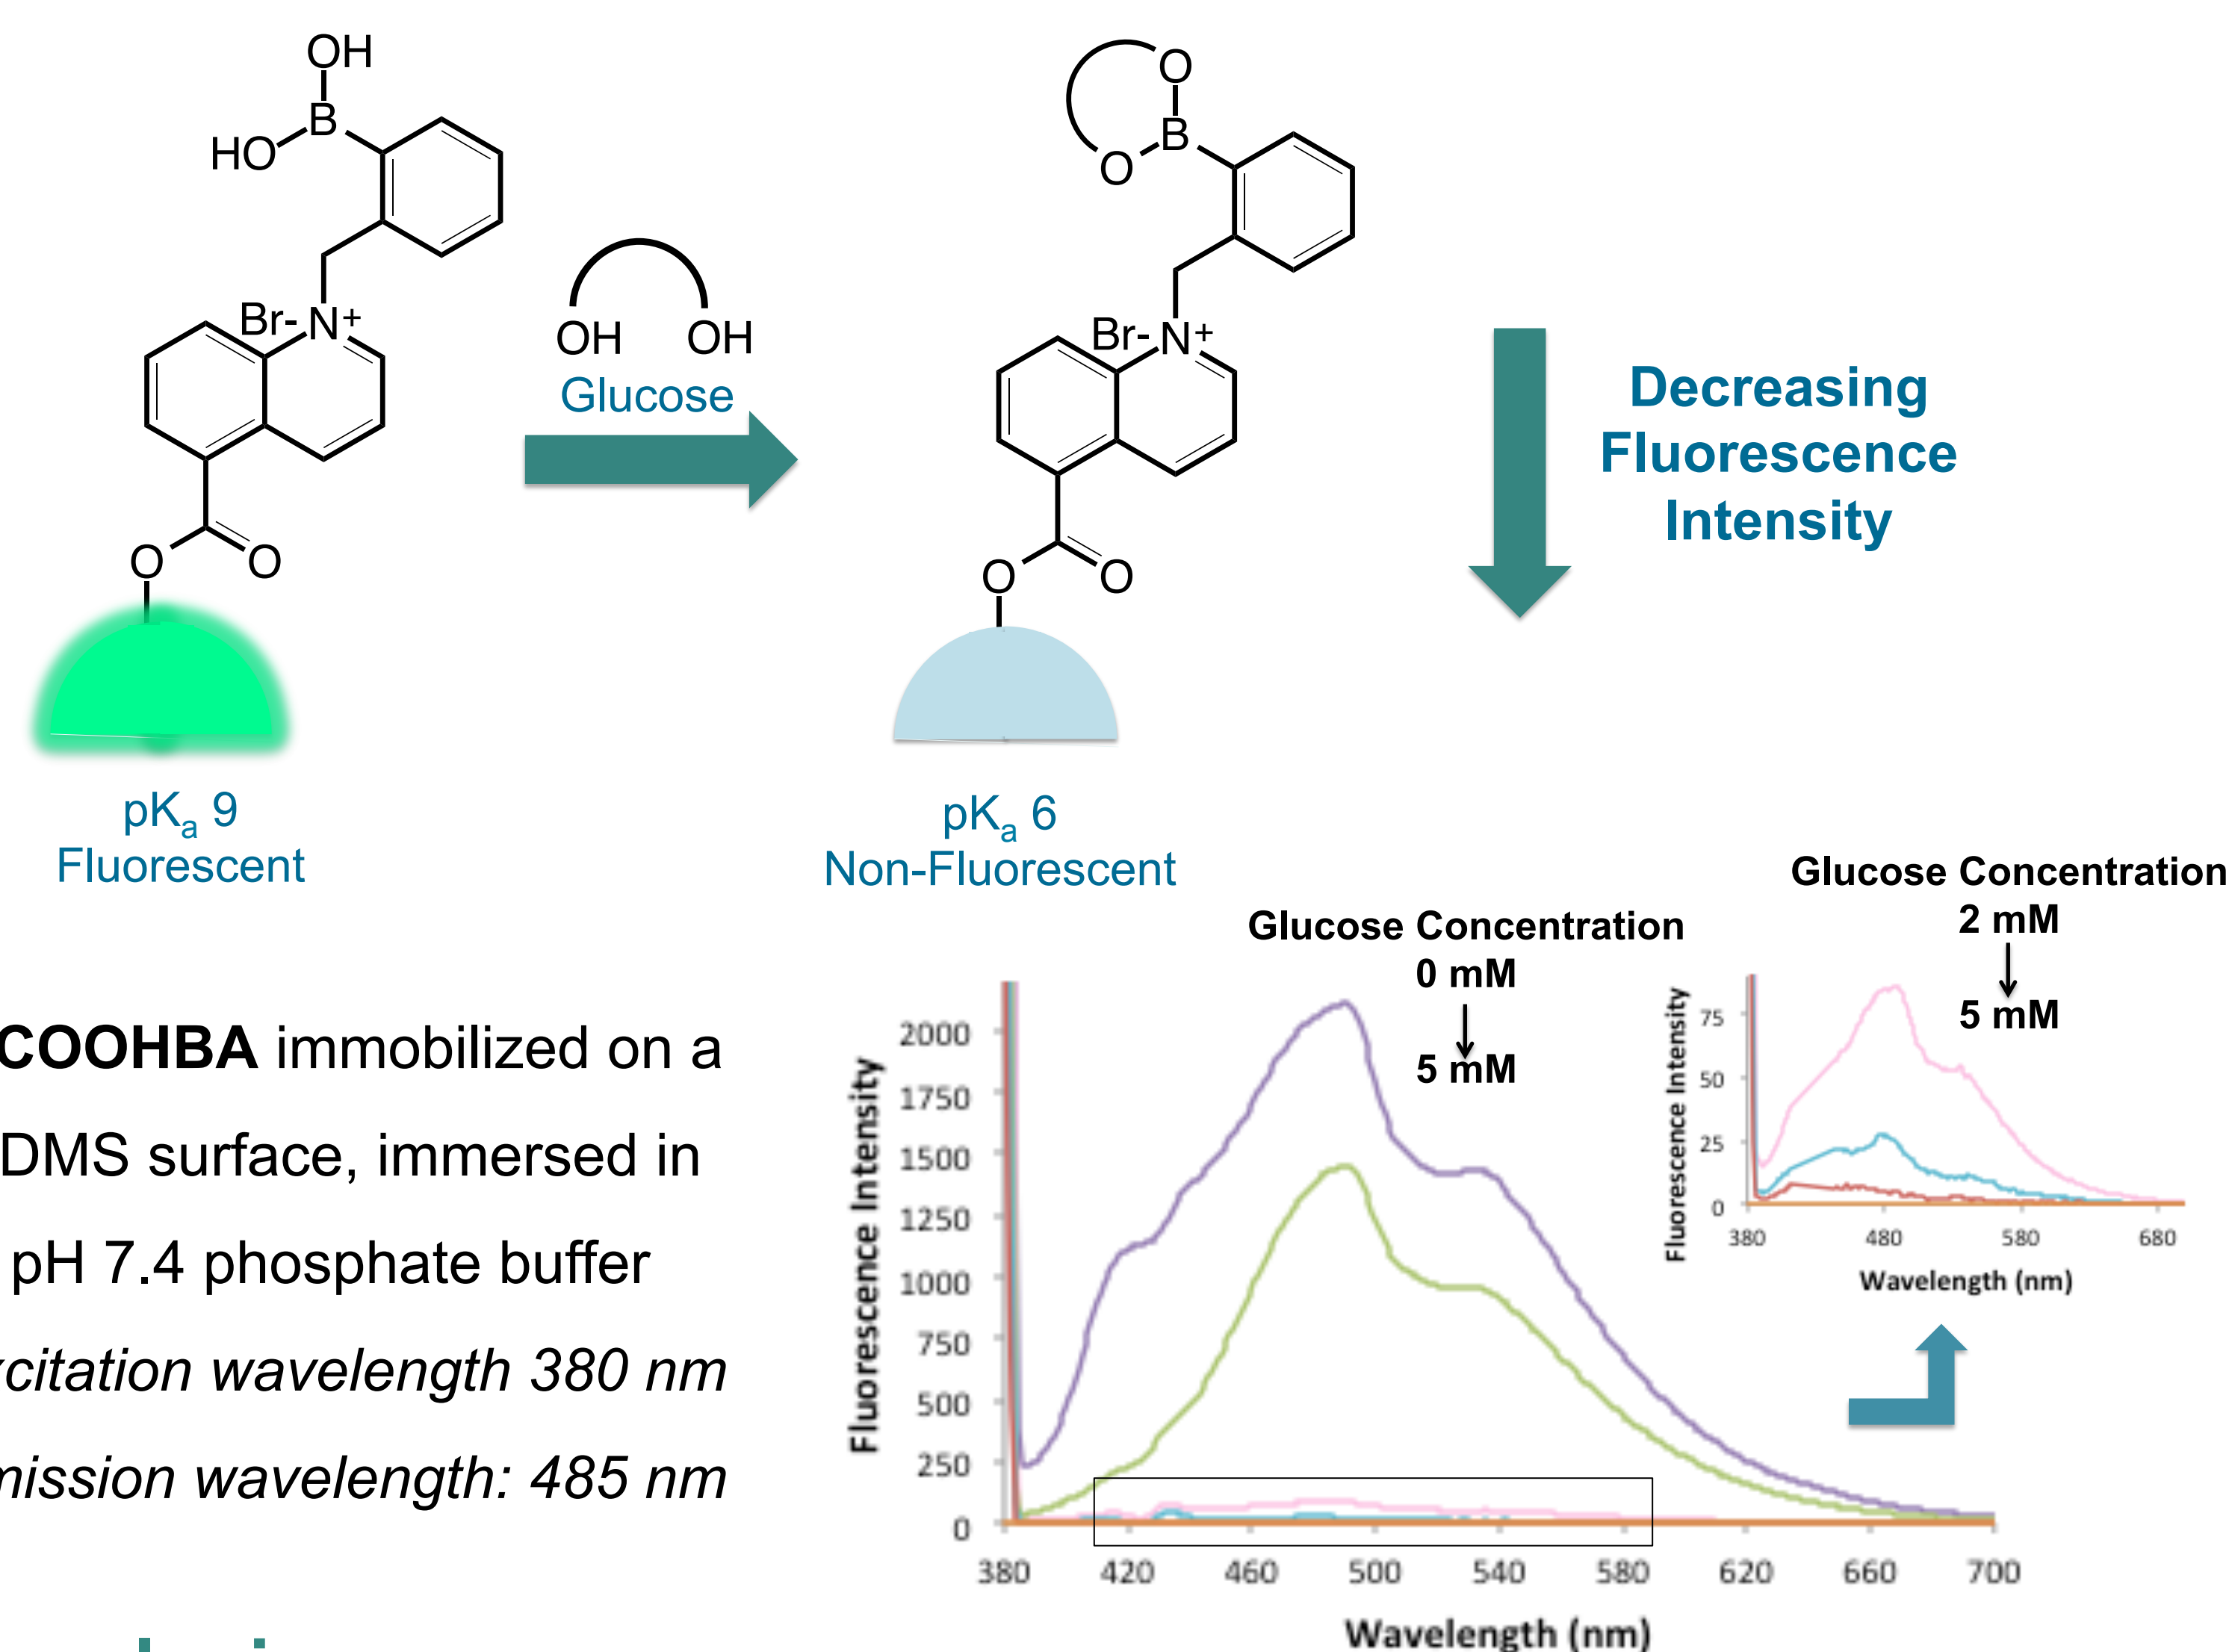

o-COOHBA immobilized on a PDMS surface, immersed in pH 7.4 phosphate buffer

Excitation wavelength 380 nm

Emission wavelength: 485 nm

Conclusions

In both solution studies and when anchored on to the PDMS surface, a decrease in fluorescence intensity was observed on increased glucose concentrations. The excitation wavelength of 380 nm is advantageous, as it lies close to the visible-region of the electromagnetic spectrum, which allows for the use of cheap, readily available LEDs as excitation sources. The large Stokes shift of 100 nm is also ideal for a sensing application. The carboxylic acid substituent was also desirable for immobilizing the BA sensor onto a wide variety of polymeric substrates.